

# FOR REFERENCE ONLY

PRODUCT SPECIFICATIONS MUST BE FILLED IN AT TIME OF ORDER:

COMPLETE PART NUMBER: \_\_\_\_\_


TORQUE SETTING: \_\_\_\_\_ ±10%

COLOR OF HANDLE: \_\_\_\_\_

APPROVAL/DATE: \_\_\_\_\_

## REVISIONS

REV	DESCRIPTION	DATE/BY	ECO NO.

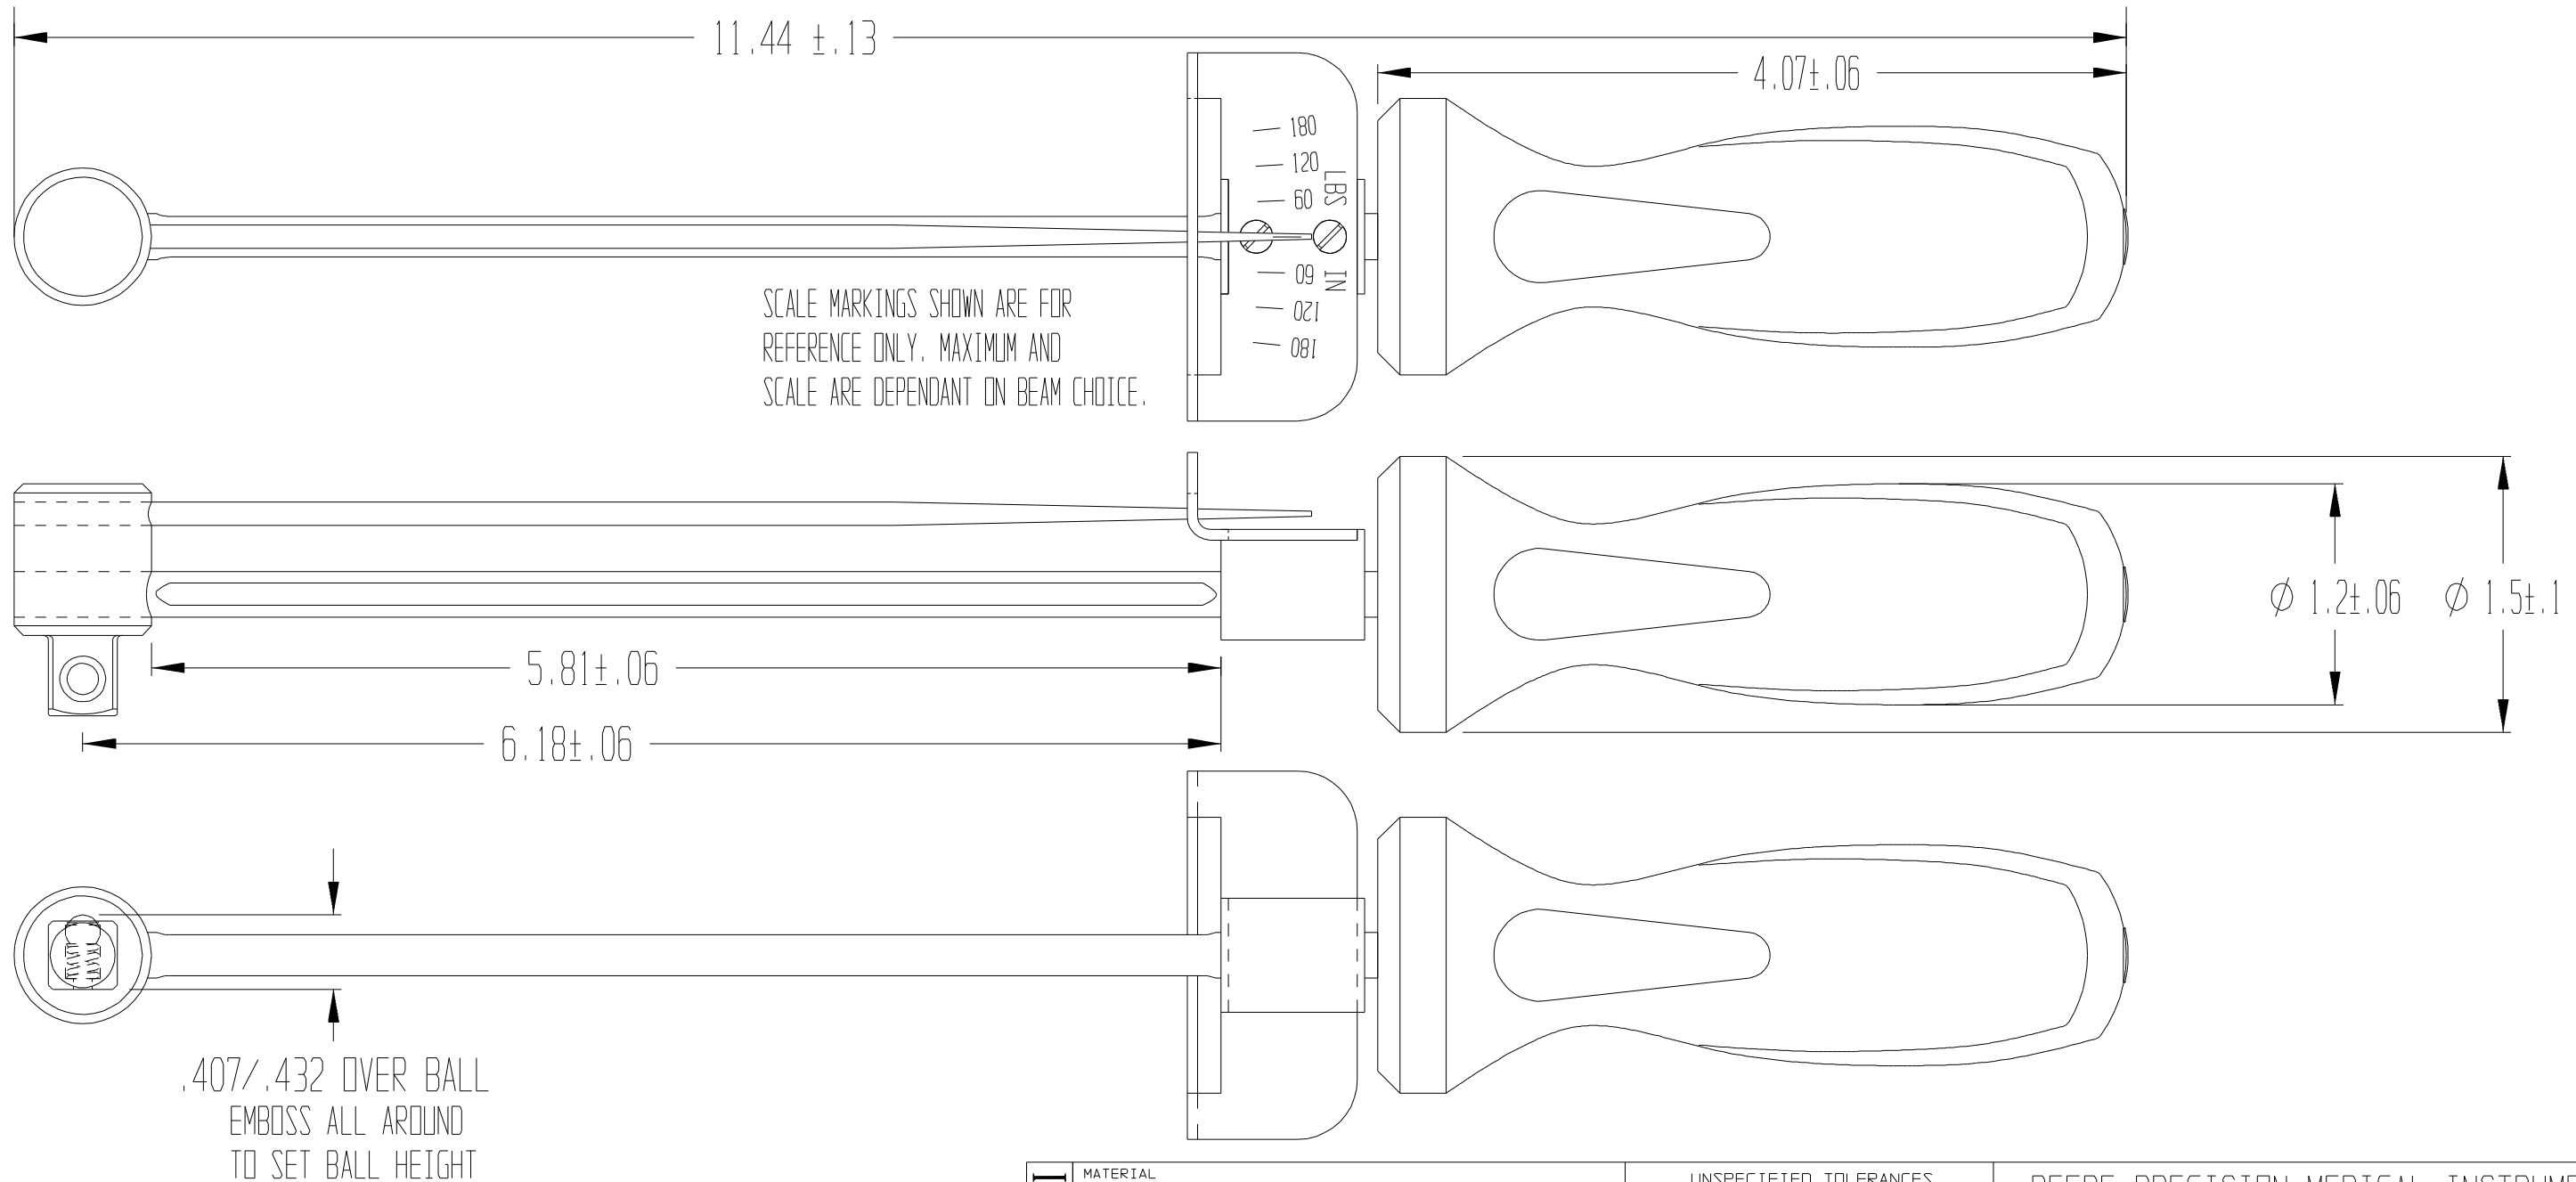

THIS DOCUMENT INCLUDING ALL DATA, SPECIFICATIONS, AND INFORMATION CONTAINED WITHIN IS CONFIDENTIAL AND PROPRIETARY TO BEERE PRECISION MEDICAL INSTRUMENTS, INC. BY RETENTION, THE RECIPIENT AGREES NOT TO REPRODUCE, DISCLOSE, OR MAKE USE OF ITS CONTENTS IN ANY WAY WITHOUT PRIOR WRITTEN PERMISSION OF AN OFFICER OF BEERE PRECISION MEDICAL INSTRUMENTS, INC.

DB101184	MATERIAL	UNSPECIFIED TOLERANCES		BEERE PRECISION MEDICAL INSTRUMENTS, INC. 2503 LINCOLNWOOD CT., RACINE WI 53403 (262) 554-8505				
	HEAT TREAT	.X    +/- .020	ANGLE    +/- 1°					
	FINISH	.XX    +/- .010	MACHINE	TITLE DEFLECTION BEAM TORQUE WRENCH 180 IN LB				
		.XXX    +/- .005	FINISH    32√					
		.XXXX    +/- .0005	CONCENTRICITY    .005 T.I.R.	DO NOT SCALE DRAWING	SIZE    B	SUPERSEDED NO.	DWG NO    DB101184	REV    G
	REMOVE ALL BURRS	BREAK SHARP CORNERS	SQUARENESS    .001 PER IN.	DATE    6/23/94	SCALE    FULL	ILLUSTRATION		SHEET    1    OF    1
	PART TO BE FREE OF DIRT, OIL, AND CONTAMINANTS			DATE				